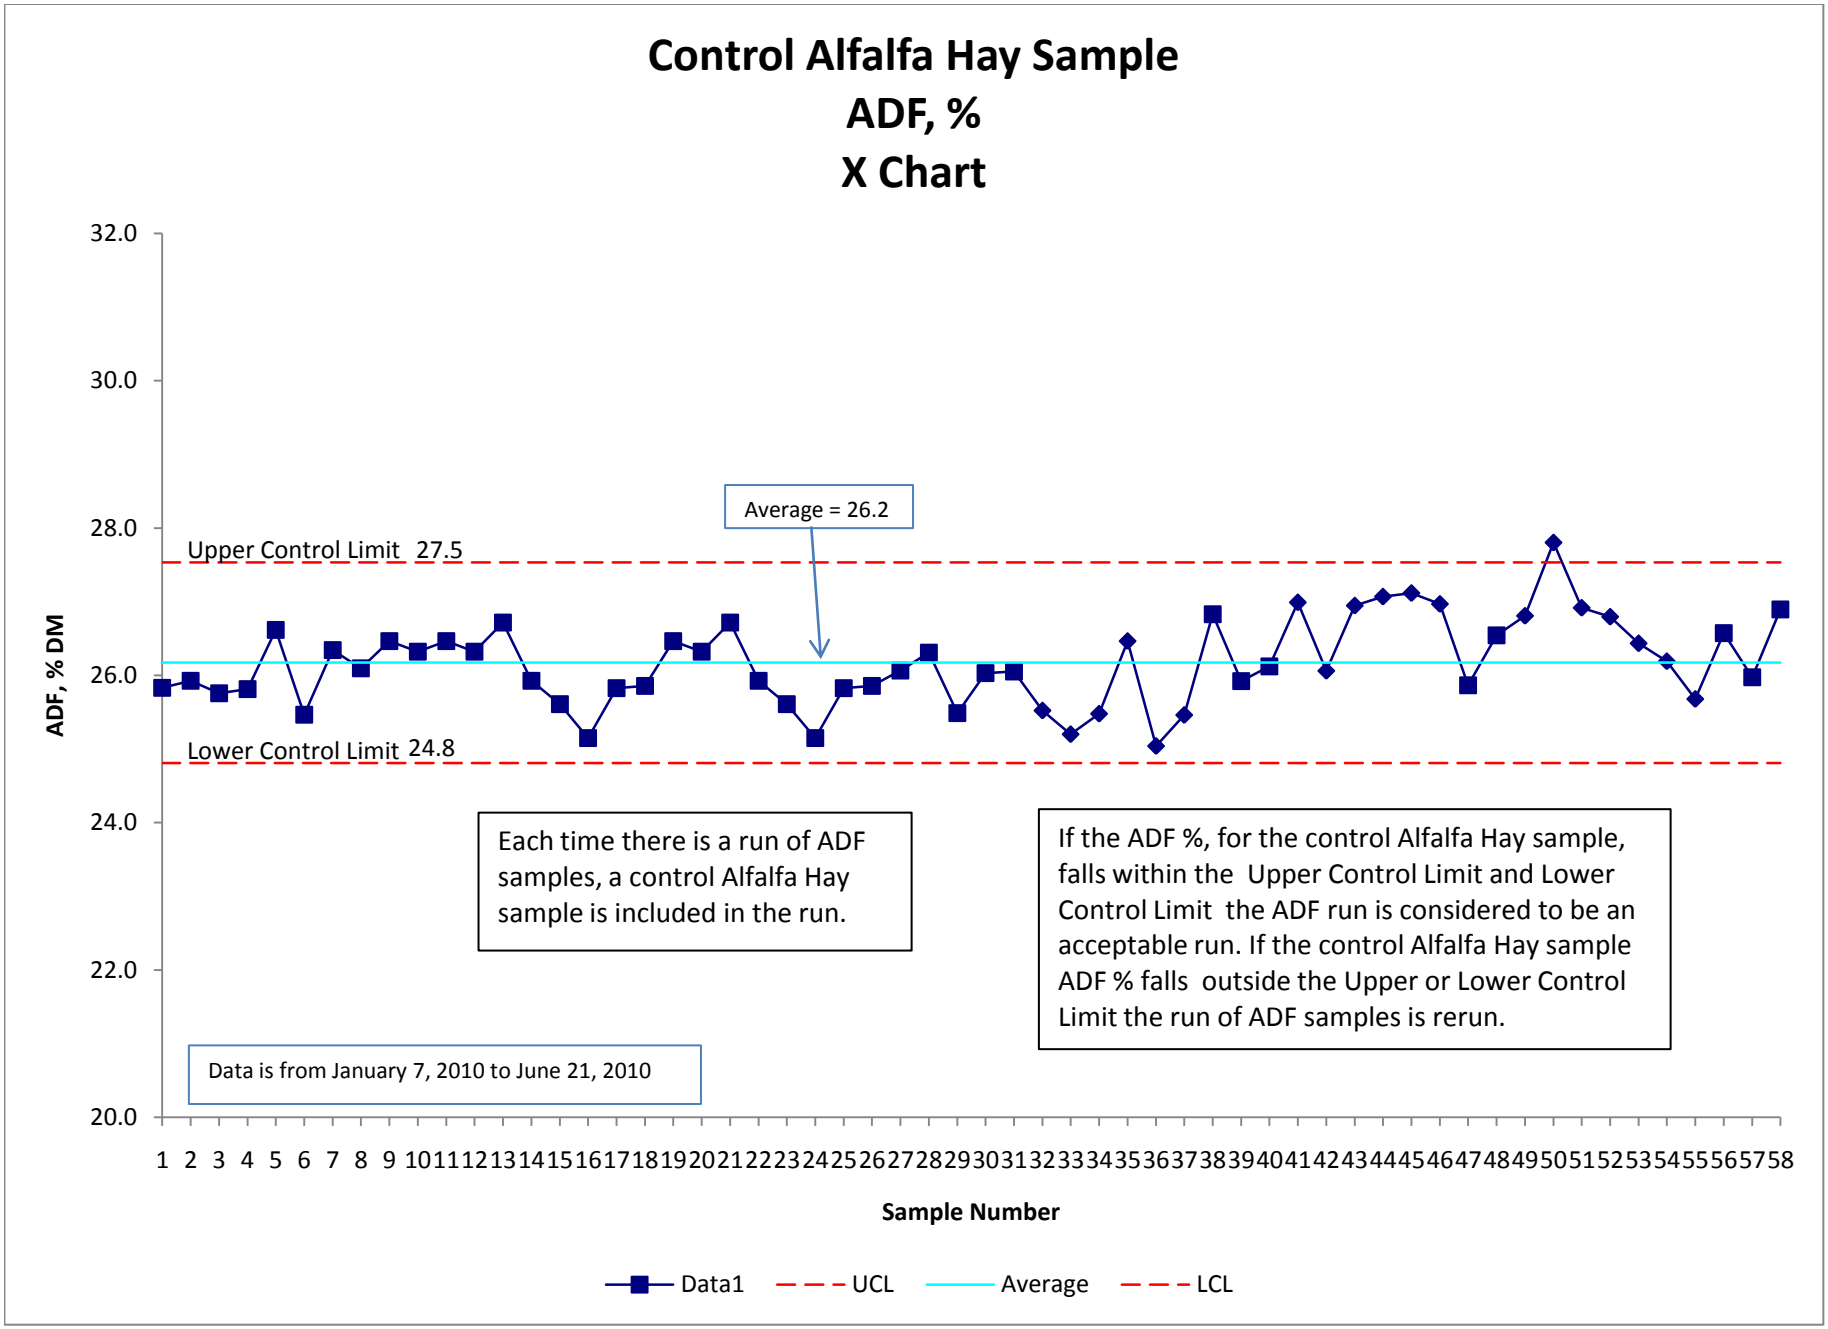
Control Alfalfa Hay Sample
ADF, %
X Chart
ADF, % DM
32.0
30.0
28.0
26.0
24.0
22.0
20.0
Upper Control Limit 27.5
Average = 26.2
Lower Control Limit 24.8
Each time there is a run of ADF samples, a control Alfalfa Hay sample is included in the run.
If the ADF %, for the control Alfalfa Hay sample, falls within the Upper Control Limit and Lower Control Limit the ADF run is considered to be an acceptable run. If the control Alfalfa Hay sample ADF % falls outside the Upper or Lower Control Limit the run of ADF samples is rerun.
Data is from January 7, 2010 to June 21, 2010
Sample Number
Data1
UCL
Average
LCL