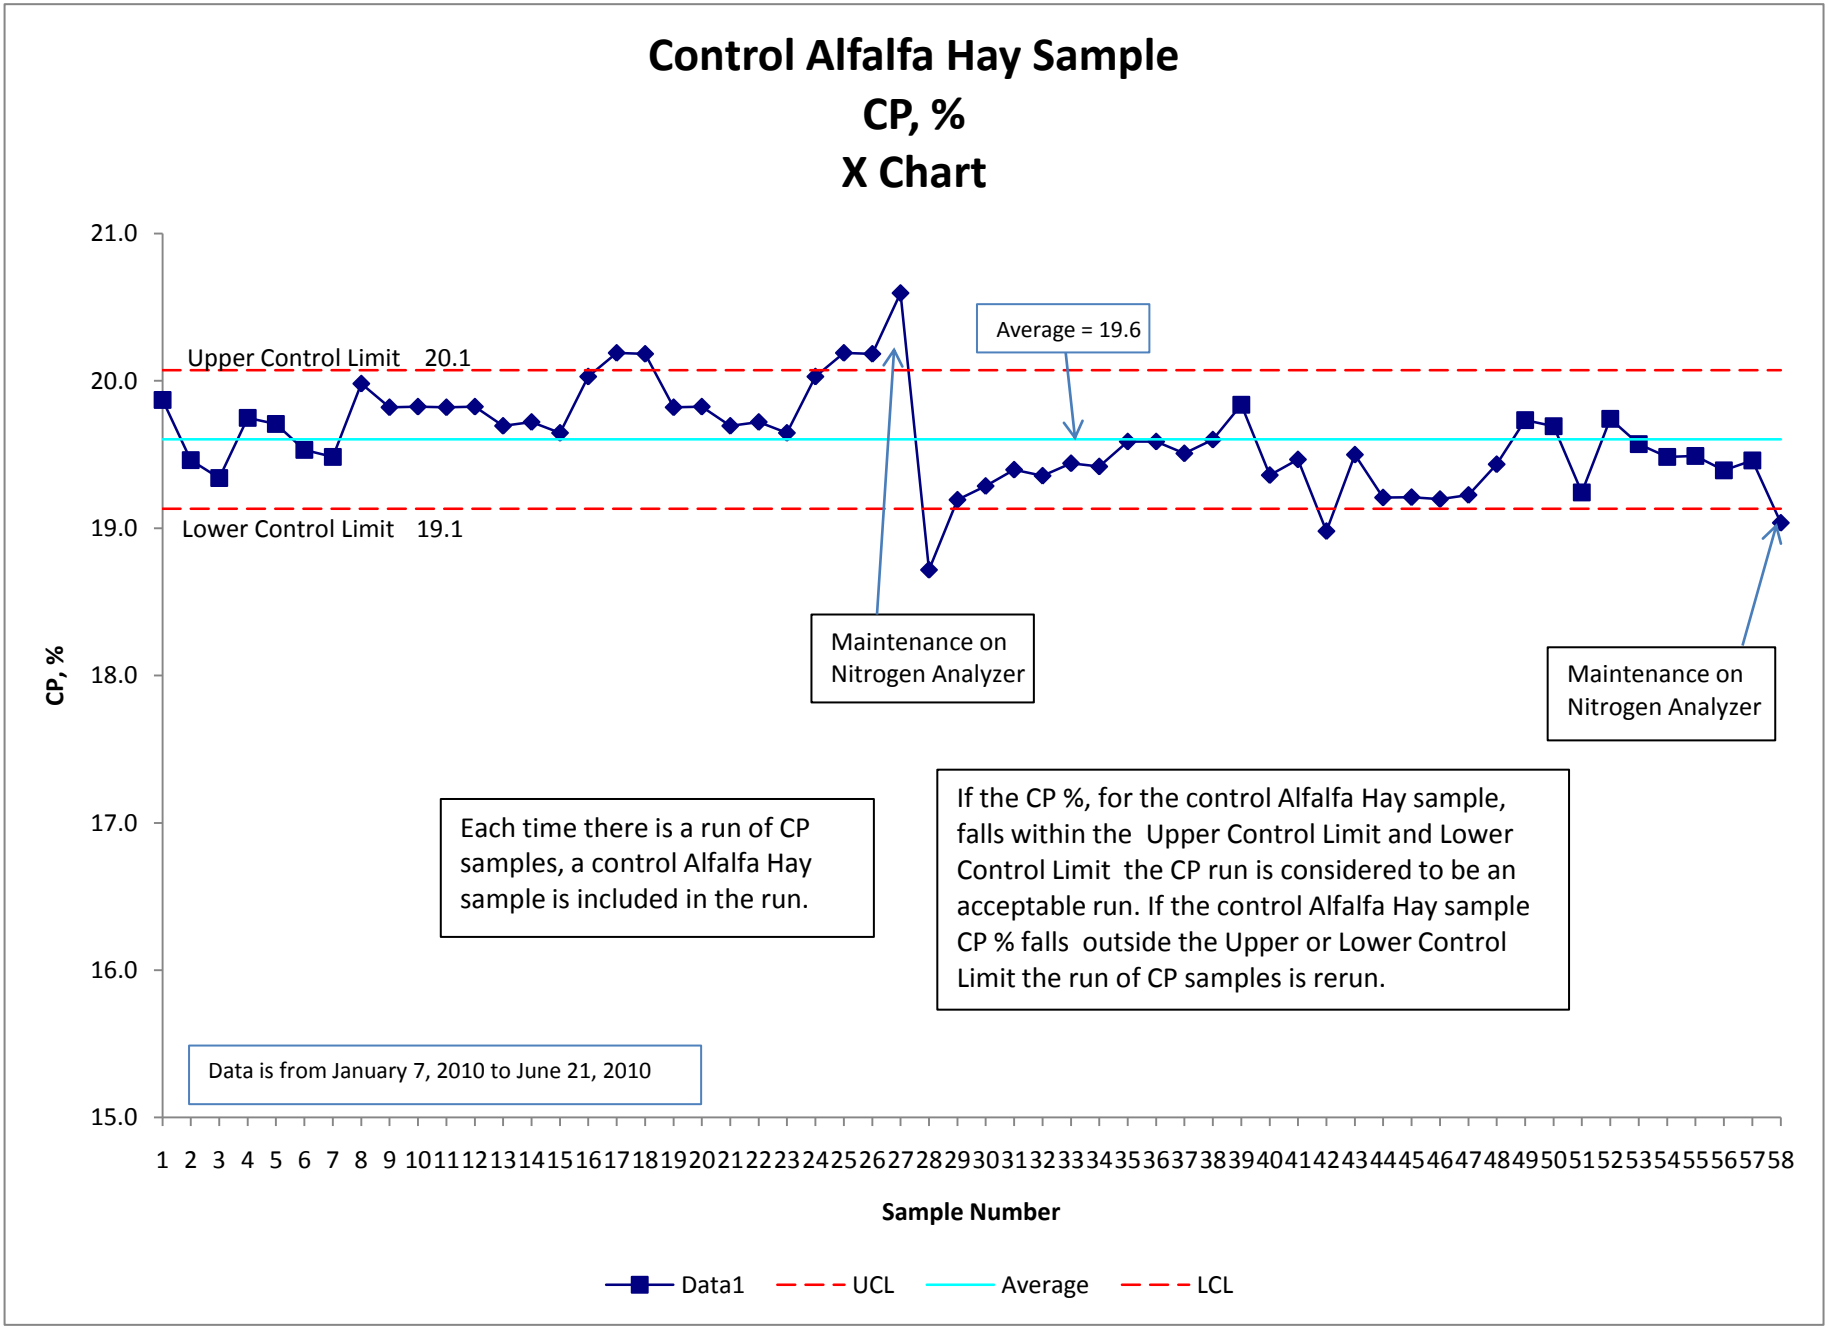
Control Alfalfa Hay Sample
CP, %
X Chart
21.0
20.0
19.0
18.0
17.0
16.0
15.0
CP, %
Upper Control Limit 20.1
Lower Control Limit 19.1
Average = 19.6
Maintenance on Nitrogen Analyzer
Maintenance on Nitrogen Analyzer
Each time there is a run of CP samples, a control Alfalfa Hay sample is included in the run.
If the CP %, for the control Alfalfa Hay sample, falls within the Upper Control Limit and Lower Control Limit the CP run is considered to be an acceptable run. If the control Alfalfa Hay sample CP % falls outside the Upper or Lower Control Limit the run of CP samples is rerun.
Data is from January 7, 2010 to June 21, 2010
Sample Number
Data1
UCL
Average
LCL