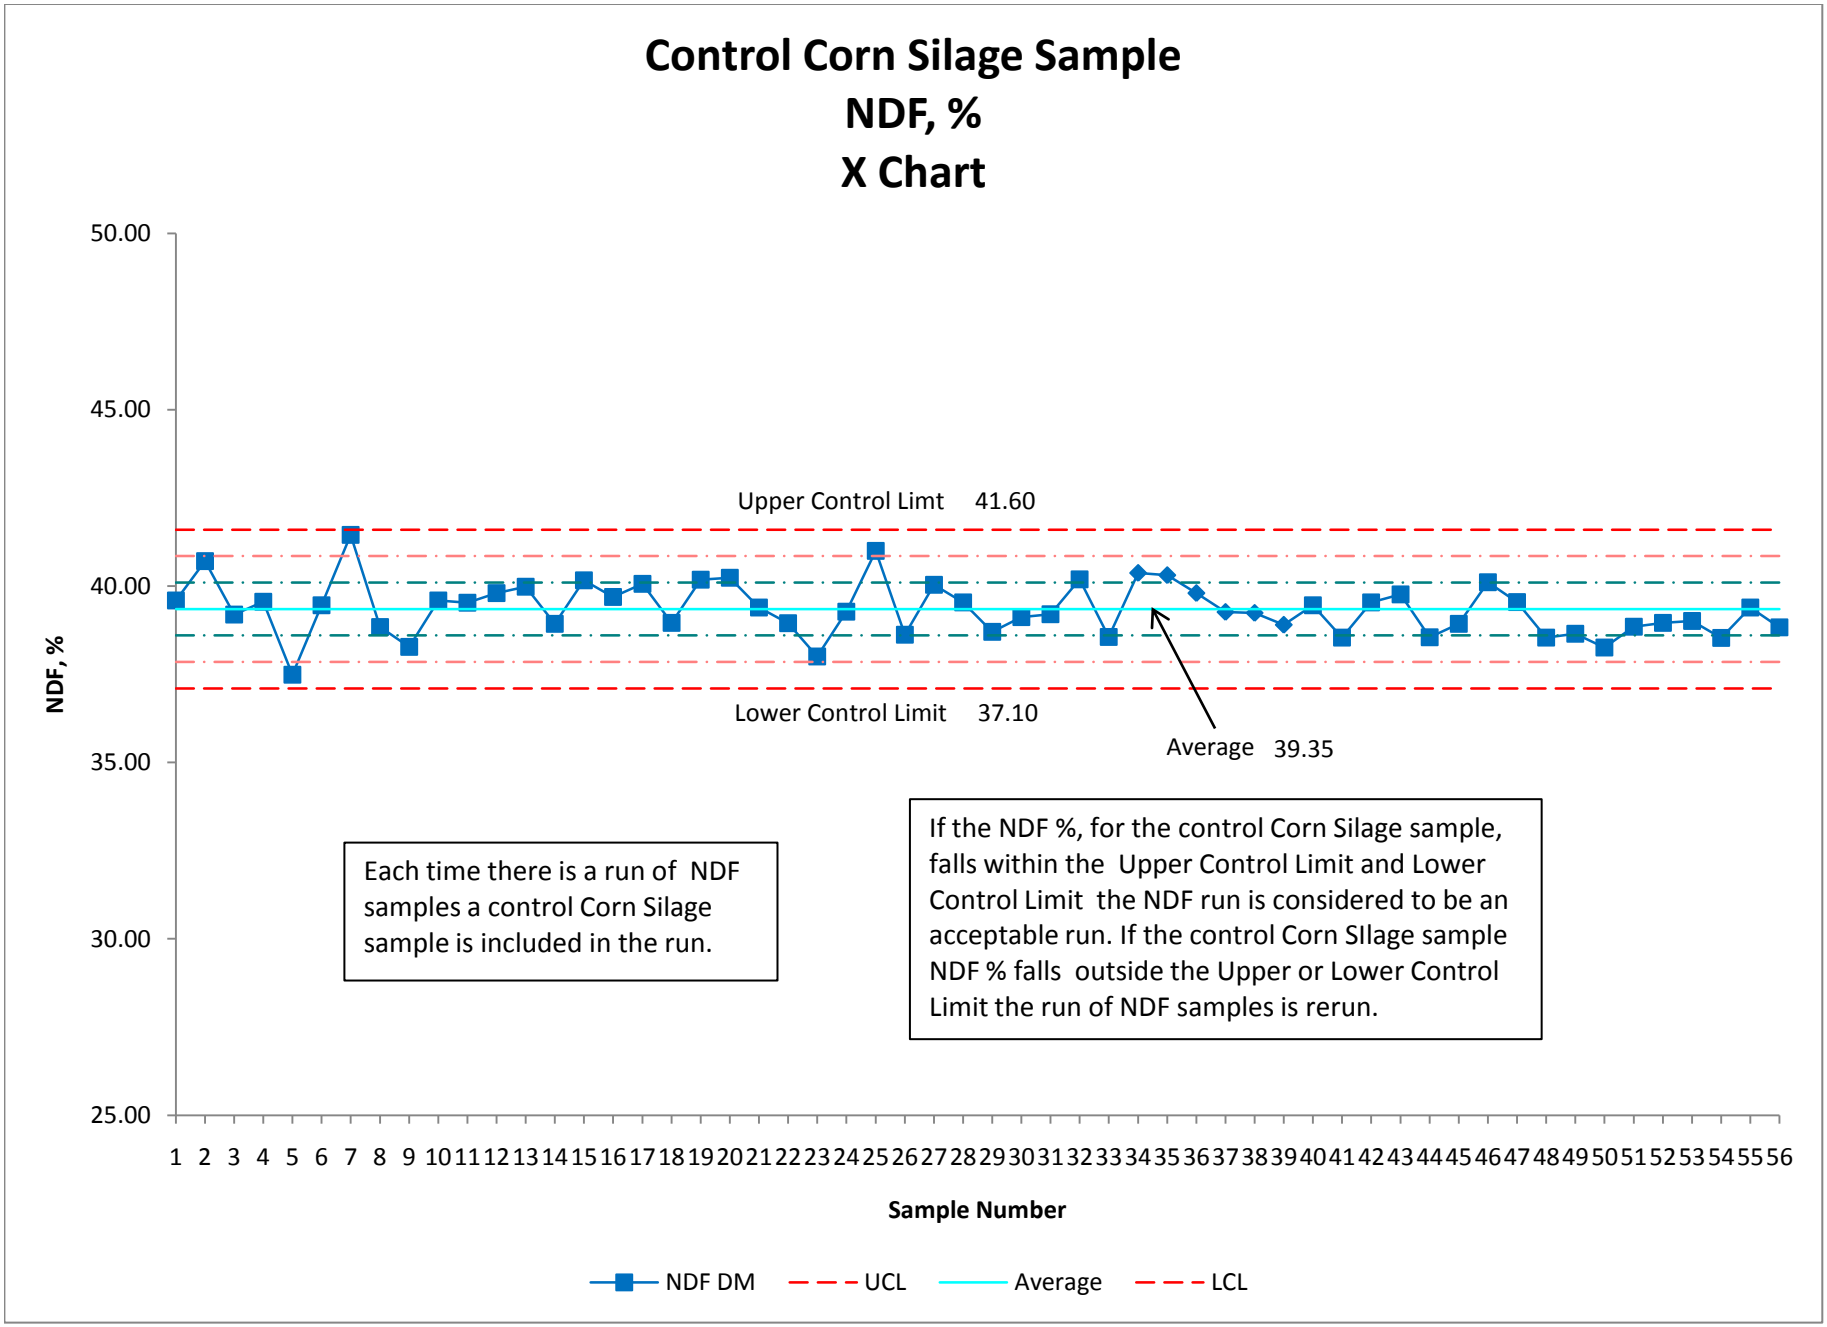
Control Corn Silage Sample
NDF, %
X Chart
50.00
45.00
40.00
35.00
30.00
25.00
NDF, %
Upper Control Limt 41.60
Lower Control Limit 37.10
Average 39.35
Each time there is a run of NDF samples a control Corn Silage sample is included in the run.
If the NDF %, for the control Corn Silage sample, falls within the Upper Control Limit and Lower Control Limit the NDF run is considered to be an acceptable run. If the control Corn SIlage sample NDF % falls outside the Upper or Lower Control Limit the run of NDF samples is rerun.
Sample Number
NDF DM
UCL
Average
LCL