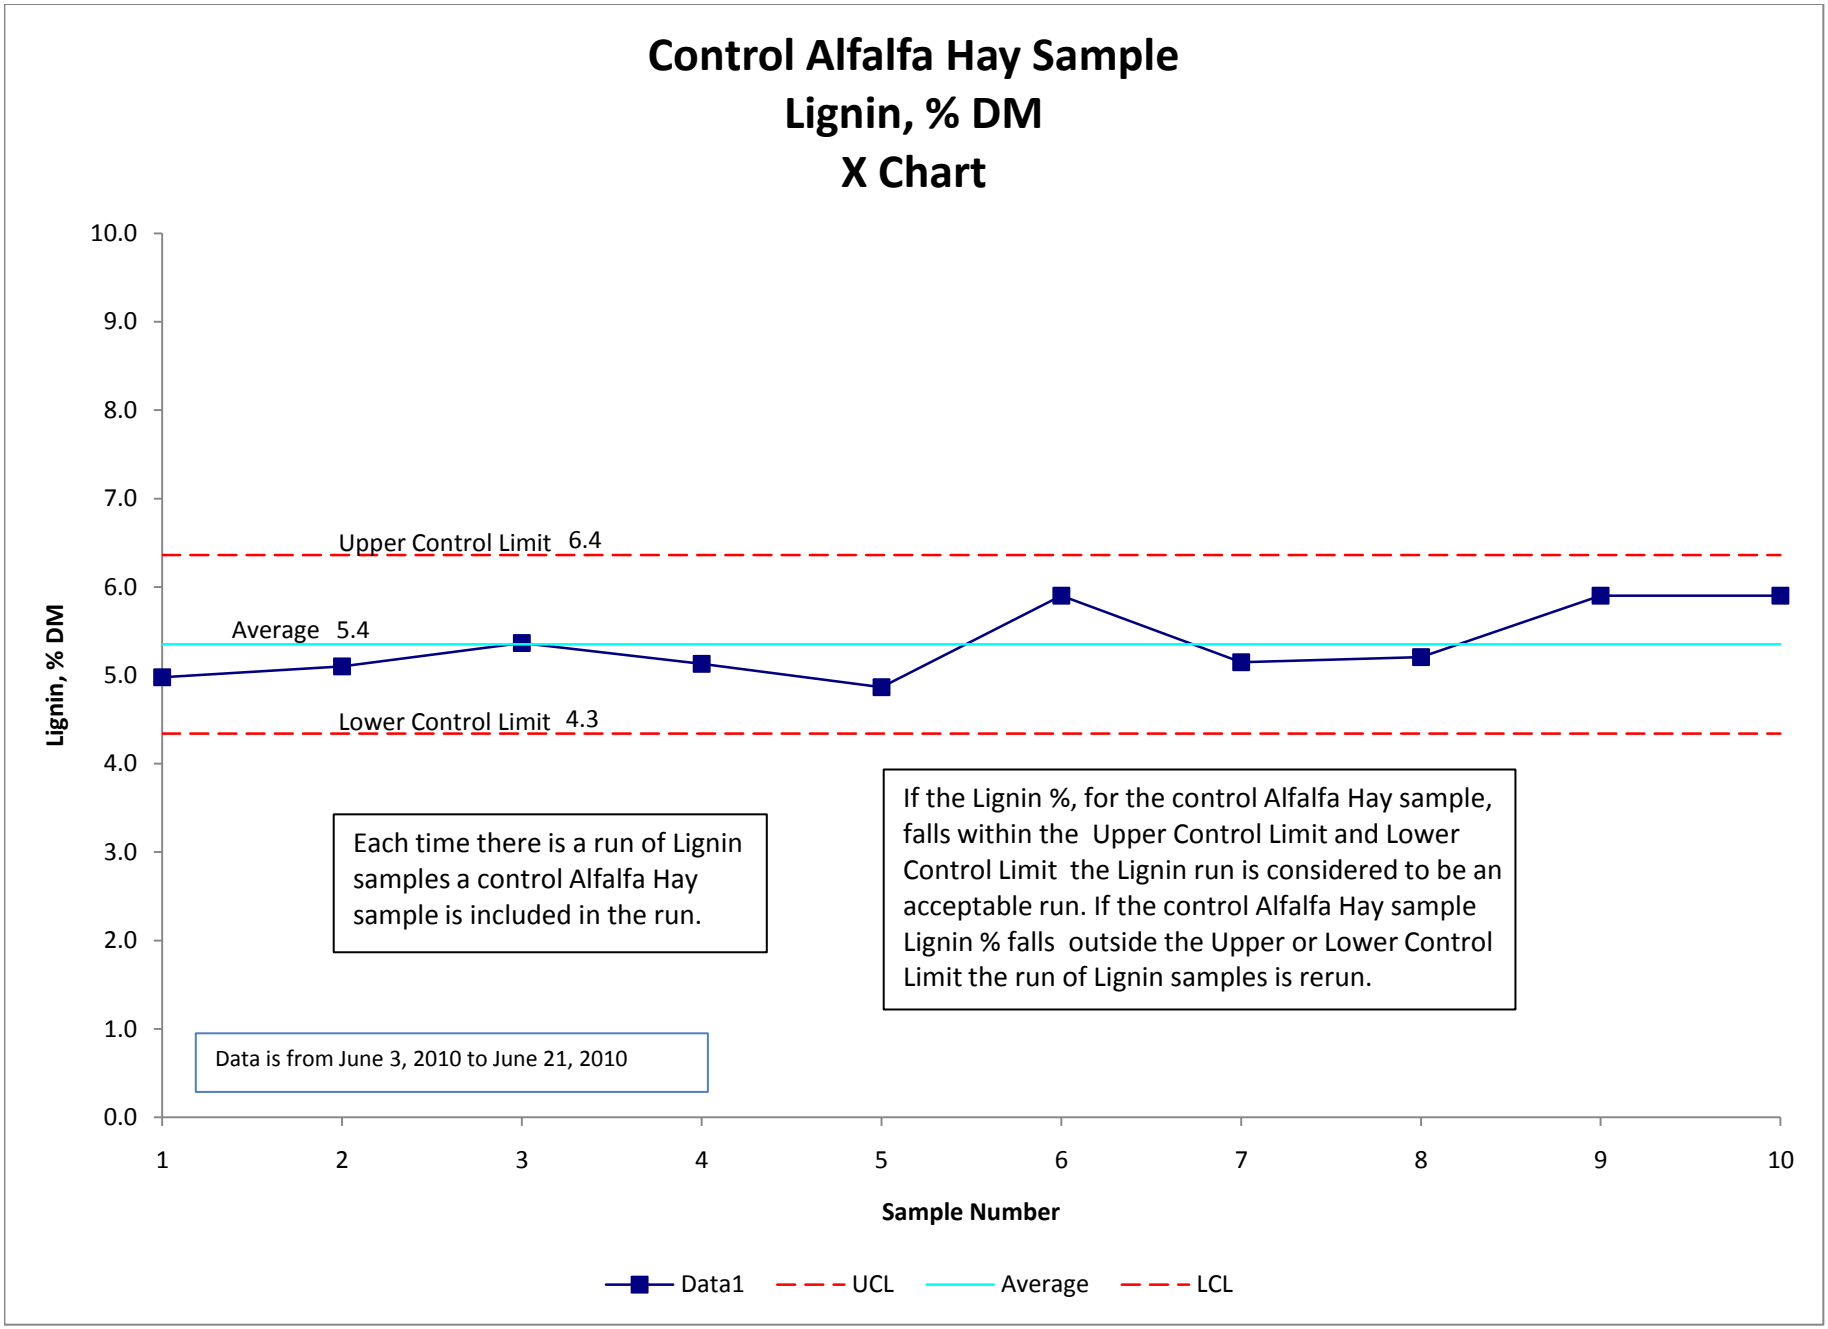
Control Alfalfa Hay Sample
Lignin, % DM
X Chart
10.0
9.0
8.0
7.0
6.0
5.0
4.0
3.0
2.0
1.0
0.0
Lignin, % DM
Upper Control Limit 6.4
Average 5.4
Lower Control Limit 4.3
Each time there is a run of Lignin samples a control Alfalfa Hay sample is included in the run.
If the Lignin %, for the control Alfalfa Hay sample, falls within the Upper Control Limit and Lower Control Limit the Lignin run is considered to be an acceptable run. If the control Alfalfa Hay sample Lignin % falls outside the Upper or Lower Control Limit the run of Lignin samples is rerun.
Data is from June 3, 2010 to June 21, 2010
1
2
3
4
5
6
7
8
9
10
Sample Number
Data1
UCL
Average
LCL